

False Positive Reduction in Lung Nodule Detection using Patch based Convolution Neural Networks

V N Sukanya Doddavarapu¹, Giri Babu Kande², B Prabhakar Rao³

¹Assistant Professor, Department of ECE, St. Ann's College of Engineering and Technology, Chirala, India, sukanyadvn@gmail.com

²Professor, ECE Department, VVIT, Nambur, 522509, Andrapradesh, India, giribabukande@gmail.com

³Professor, ECE Department, JNTUK, Kakinada, 533003, Andrapradesh, India, drbprjntu@gmail.com

Corresponding Author: First

ABSTRACT

Lung cancer is the leading disease among all the types of cancers in the world. Early prediction and diagnosis of lung cancer will increase the endurance rate of the affected patients. Therefore, in this paper, we proposed an efficient Computer-Aided Diagnosis (CADe) system for the automatic detection of pulmonary nodules and the reduction of false positives per scan from lung Computed Tomography (CT) images. Major steps in the design of the CAdE system includes preprocessing of lung slice using Riesz filter banks, image segmentation using iterative thresholding approaches, nodule detection using morphological operators. The challenging task in the design of the CAdE system is the reduction of false positives per scan. Here a novel patch-based Convolutional Neural Networks (CNN) are designed with three Convolution Layers with the number of filters as 32, 64, and 128 respectively, two maximum pooling layers, Leaky ReLU activation function to increase the process of convergence during training. The final Fully-Connected (FC) layer produces two outputs as nodule and non-nodule. After detecting pulmonary nodules 64×64 patches are drawn, which are given as inputs to CNN. The proposed method is evaluated on the publicly available huge LIDC-IDRI database. Out of 1018 cases in our study, 888 scans containing 1186 nodules are considered. The results of our proposed CAD system show biased performance giving 94.8% sensitivity and 2.8 FP/scan compared to the state-of-the-art.

Index Terms- Computer-Aided Diagnosis (CADe) system, Computed Tomography, Lung Nodule, Convolutional Neural Networks (CNN), False Positive Reduction.

1. INTRODUCTION

Cancer is a significant general medical issue overall [1]. Lung malignancy is the main source of disease passing with the most noteworthy grimness and mortality among the people in China [3]. Both males and females but more in males who undergo smoking eventually majorly affect it. It will start first in the lungs and even spread to the other organs of the body. According to the survey made by the American Cancer Society (ACS), 78% of the people are dying because of the failure of the prediction of Lung cancer in the early stages and the survival rate improved if we predict five years earlier [4]. Early symptoms include are shortness of breath, cough, chest pain, and weight loss. Many diagnosis tools in the real-time processing of lung cancer are Computed Tomography (CT), Magnetic Resonance Imaging (MRI), and Positron Emission Tomography (PET). Among these Computed Tomography (CT) imaging is widely used because of its cost-effectiveness and also the mortality of Lung Cancer decreased by 20%. The early prediction of Lung Cancer dependent on low dose Computed Tomography (CT) imaging gives good results for further treatment of the lung cancer affected patient.

Pulmonary Nodule also called Rounded Opacity has a diameter up to 3cm when measured on Chest [6]. Pulmonary Nodules are classified based on internal texture as solid, part-solid, and non-solid, based on location as juxta-pleural, juxta-vascular, and well-circumscribed as shown in Fig. 1.

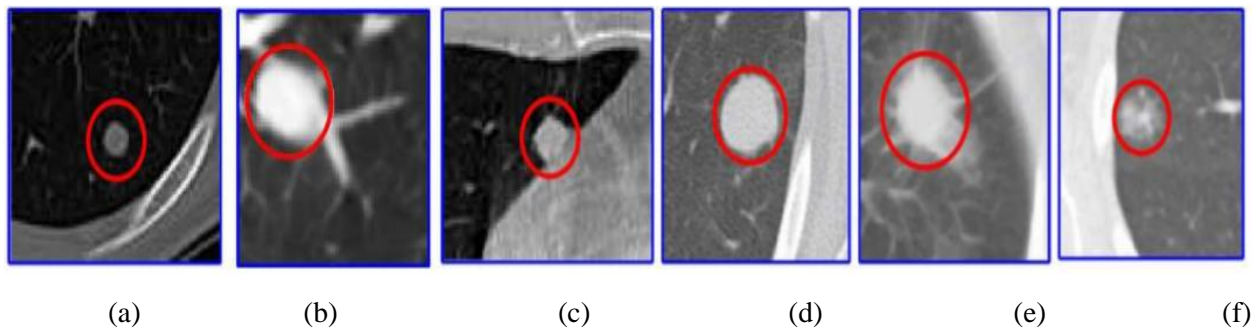


Fig. 1 The visual aspect of different types of Pulmonary Nodules: From left to right Well Circumscribed, Juxta-Pleural, Juxta-Vascular, Solid, Part-Solid, and Non-Solid.

It is the task of the radiologists to determine the malignancy of the Lung based upon the shape, size, and texture of the Pulmonary nodule for further treatment. Even for trained radiologists, it is difficult to interpret when they are in heavy workload. As a result, a computer-aided diagnosis system is needed for the automatic detection and diagnosis of pulmonary nodules. Therefore, in this paper, we propose an efficient CADe system for the detection of the pulmonary nodules of type Solid, Sub-solid, and Large Solid nodules and false positive reduction using patch-based Convolution Neural Network (CNN).

2. RELATED WORK

Many CAD systems are designed for the detection and diagnosis of pulmonary nodules. In general, CAD systems are classified into two types: Computer-Aided Detection (CADe) systems and Computer-Aided Diagnosis (CADx) systems. CADe systems are used to detect nodules, segment, and reduce False Positives, whereas CADx systems are used to classify the lesion into Benign or Malignant. In the present work, we focus on CADe systems for the early detection of the Pulmonary nodules and to reduce the False Positive (FP)/scan. The main steps include 1) Lung Slice Pre-processing, 2) Lung Segmentation, 3) Lung Nodule Detection, and 4) False Positive Reduction. Most of the preprocessing techniques include contrast stretching [22], Discrete Wavelet Transform (DWT) [25], masking and isotropic resampling [26], Hough transform [35], smoothing filter [31], median filter [33], morphological hole filling operator [31], erosion filter [24], linear transformation [15], and thresholding [17]. The most popular lung segmentation algorithms that yields better nodule detection include morphological filters [16,22,27], region growing [29], OTSU thresholding method [13,15], fuzzy C-means clustering [25], edge detection [30], active contour models [10,15,17]. Major stage of this work includes nodule detection, thresholding and clustering [19,26,28], statistical region merging [23], spatial fuzzy c-means (SFCM) [12], 3D detection box [23], CNN's [9,21]. The tough task is False Positive (FP) reduction, which includes assortment of different features extracted for better classification results. Based on types of the features intensity [13,22,26,27], geometry [13,26,27] and texture [34]. Recent works include gradient features [27], metabolic features [32], and spatial context [26]. Based on the classifier SVM [20,26,27,28], Rule-based method [22,27], ConvNet [19], and Particle Swarm Optimization (PSO) [2].

3. METHODS

Most of the medical images contain some redundant data at high-level frequencies during image acquisition that can be removed by proper processing techniques. In this section, we will discuss in detail the different stages of the CADe system as shown in Fig. 2.

Lung Slice pre-processing

The first stage after acquiring the lung Slice from the dataset is pre-processing. The Lung Computed Tomography (CT) image in general consists of some unwanted components along with the relevant data because various artifacts such as noise, motion, variations, shift, and non-uniform intensity affect the image quality. Hence preprocessing is the important step for removing unwanted components keeping useful data. Here in the present work Riesz filters [5], are used for the enhancement of lung boundaries.

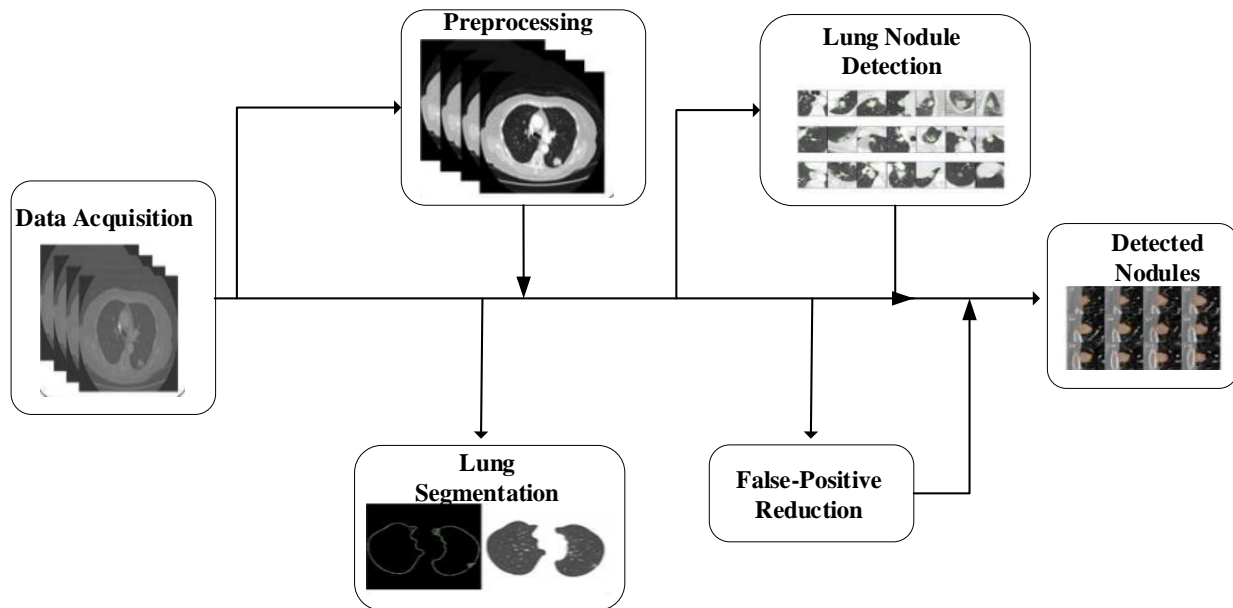


Fig. 2. Flow diagram of the proposed CADe system

Image Segmentation and Nodule Detection

The next stage followed by image preprocessing is image segmentation that consists of numerous methods in the literature. As shown in Fig. 3 the lung CT image consists of fat, bones, muscles, etc. To extract the lung region we have to select proper threshold value.

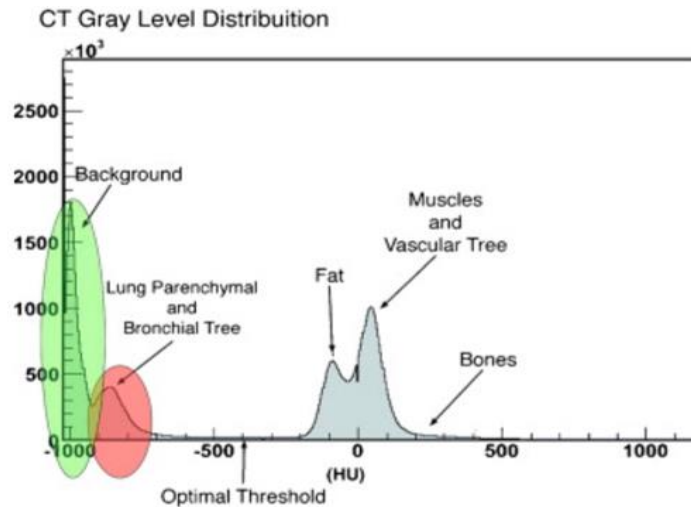


Fig. 3 Histogram of the Lung CT gray-level distribution

Clearly, from the histogram low-intensity values corresponds to lung region, and high-intensity values correspond to fat, muscle, bones, etc. To solve this problem an iterative threshold-based technique [10] is proposed in this paper. After thresholding, by using morphological closing operation nodules are detected.

Patch Extraction

From the detected lung nodules 2-Dimensional image patches are extracted with a resolution of 0.78mm similar to the resolution of the CT lung slice. Initially, the image patches are drawn from 50×50 mm size and next converted into 64×64 pixels with intensity range rescaled to (0,1). To extract the patches a cube of size $50 \times 50 \times 50$ is considered enclosing the nodule detected to the center of the cube. Nine patches are drawn in axial, sagittal, and coronal planes as in [7].

False-positive Reduction

It is a challenging step in any type of CAD system to reduce the false-positive rate. The true pulmonary lung nodules appear in different shapes and sizes whereas the false pulmonary lung nodules appear similarly as shown in Fig. 4. To solve this problem we provide a 2-dimensional Convolutional Neural Network (CNN) architecture for reducing the false positive rate.

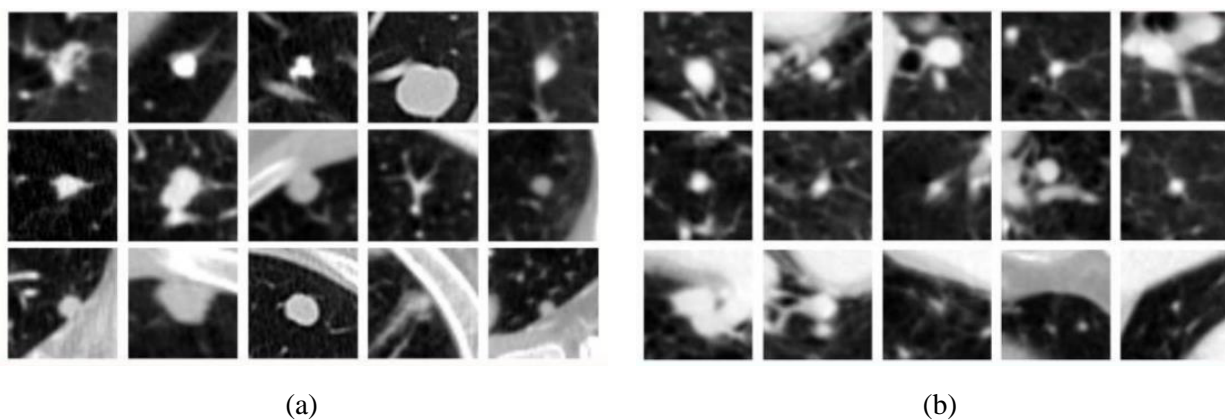


Fig. 4 Visual aspect of lung nodules a) True positive nodules b) False-positive nodules.

The input to the CNN is 64×64 patches drawn from the lung nodules detected in the previous step. The architecture for the assortment of features for the classification of pulmonary nodules as non-nodule and nodule is as shown in Fig. 5.

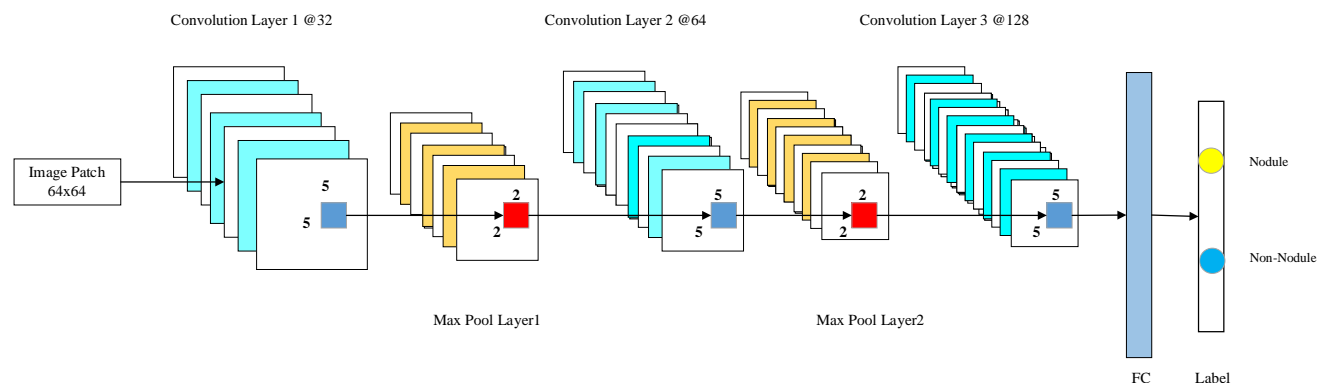


Fig. 5. Patch based CNN architecture for false-positive reduction

The architecture consists of three convolution layers with kernels of size 5×5 with stride 1, and the number of filters as 32, 64, and 128 respectively. The convolution layers are followed by a max-pooling layer with kernels of size 2×2 with stride as 2. For speeding the process of convergence during training Leaky ReLu activation layer is used. The output feature maps are connected to a softmax layer with a dropout of 0.5%. Data Augmentation using translation method is performed to only nodules patches, as they are fewer in number compared to non-nodules patches. The training of CNN is done by minimizing the loss function with Adam optimizer with zero bias, minimum batch size as 64, initial learning rate as 0.001, and the number of epochs as 20.

4. MATERIALS

The proposed CAD system is executed on the publicly available Lung Image Database Consortium (LIDC-IDRI) database. In the database, 1018 cases are taken from four radiologists in two rounds. For the CT images, the slice thickness varies from 0.6mm to 5mm. The images are available in DICOM format with 512×512 size. A separate XML sheet is provided for the number of nodules annotated by the radiologists. In the blind round, the radiologists annotated the nodules as two categories: non-nodule for nodule < 3 mm and nodule > 3mm. In the database total number of lesions that received a "nodule >= 3mm" mark from at least one of the four LIDC radiologists is 2669 and the total number of lesions that received a "nodule < 3mm" mark from at least one of the four LIDC radiologists are 4702. In the present study, only 888 scans are considered containing 1186 nodules. To evaluate the proposed CAde system the performance metrics sensitivity and False Positive per scan are used. Sensitivity is defined as in equation (1).

Sensitivity: It is defined as the ratio of the correctly predicted cases per class to the total actual cases per class.

$$sensitivity = \frac{TP}{TP + FN} \quad (1)$$

Where TP- True Positive (Nodule is predicted correctly), FP- False Positive (Non-nodule predicted as Nodule), TN- True Negative (Non-Nodule is predicted correctly), and FN- False Negative (Missed Nodule) .

5. RESULTS AND DISCUSSIONS

The proposed CADe system is assessed on the LIDC-IDRI database considering 888 scans. The number of nodules is 1186 in the given scans. On fivefold validation, the system achieved a sensitivity of 94.8%, and the number of false positives per scan is 2.8.

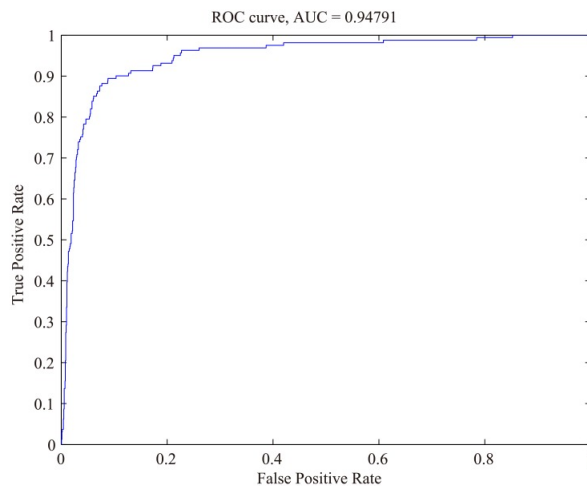


Fig. 6. ROC curve showing an AUC value of 0.94791.

The graph drawn between False Positive Rate and True Positive Rate is as shown in Fig. 6, it measures an AUC value of 0.94791. Fig. 7 shows nodules detected in a red circle using the proposed method.

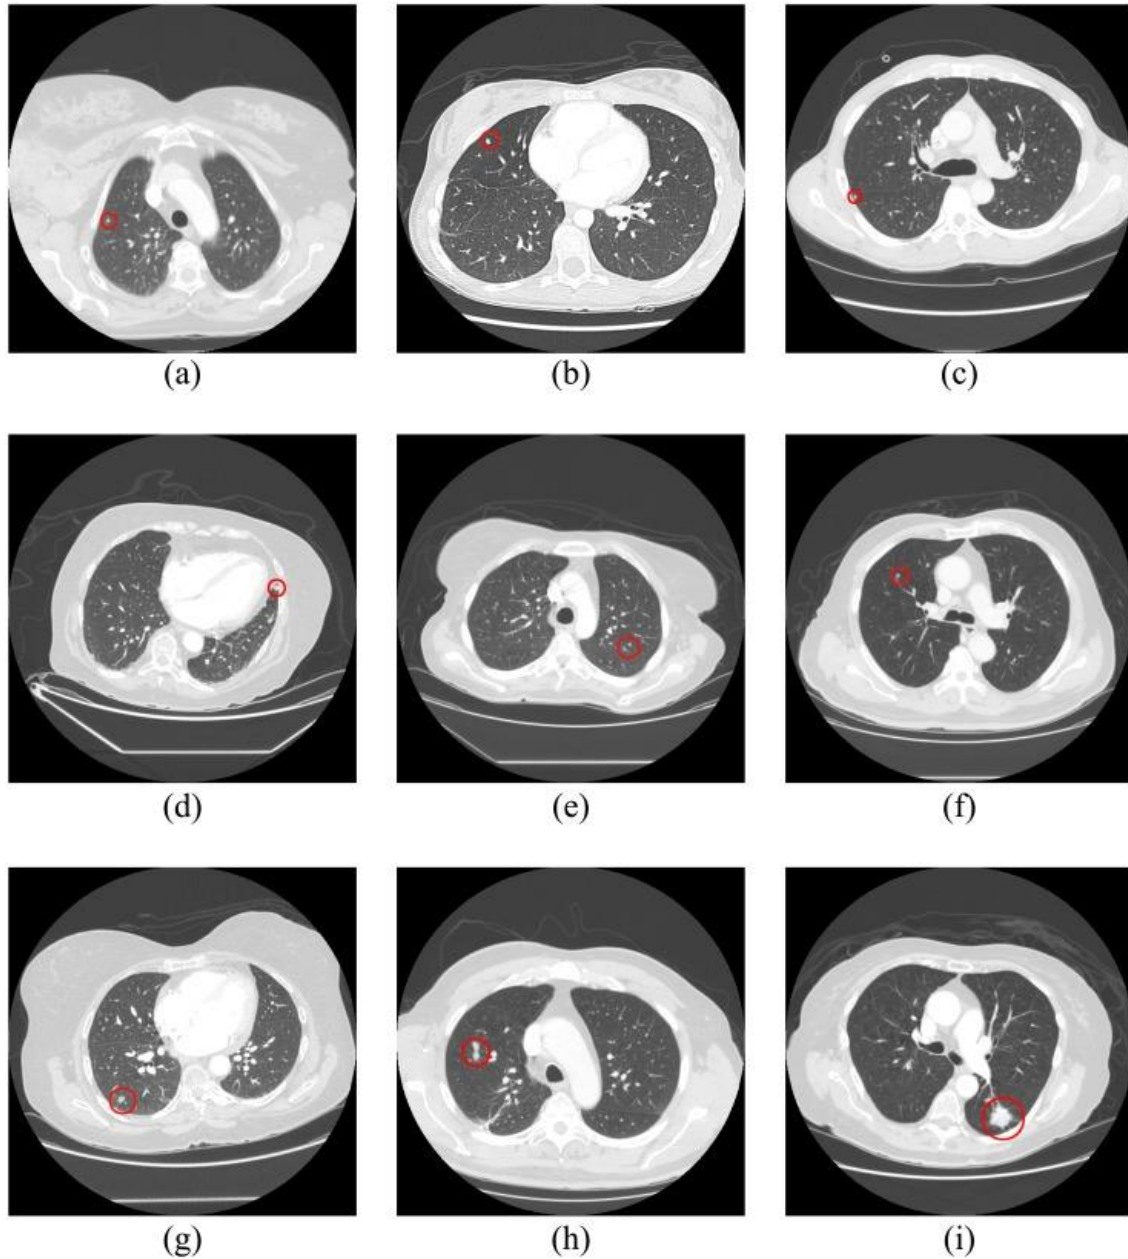


Fig. 7. Nodules detected using the proposed method.

Comparison with the recent handcraft techniques from the literature

In this section, we compare the proposed CAD system with the recent existing techniques in terms of Sensitivity, False Positives per scan, types of the database used, and the number of nodules as given in Table 1. Gong [13], detected nodules using multiscale 3D tensor filtering approach and extracted altogether 422 2D, 3D features. Out of which only 19 features are considered and given to random forest for classification. The system is evaluated on LUNA16, ANODE09, and attained a sensitivity of 79.3% and 84.62% respectively. Gupta [8], identified nodules based on multi-thresholding and morphological operation and extracted altogether 515 features and fed to the classifier to reduce false positives. This

method attained a sensitivity of 85.6% when evaluated on the LIDC-IDRI database considering 1390 nodules.

Table 1. Comparison of the proposed method with recent handcraft techniques from literature

Author	Database	No. of Nodules	Sensitivity%	FP per scan
Gong [13]	LUNA16	1186	79.3	4
	ANODE09		84.62	2.8
Gupta [8]	LIDC-IDRI	1390	85.6	8
Zhang [10]	LIDC-IDRI	168	89.3	2.1
Saien [14]	LIDC-IDRI	198	83.98	3.9
Liu [12]	LIDC	978	92.4	4.5
Proposed	LIDC-IDRI	1186	94.8	2.4

Zhang [10], segmented nodules using active contour model, nodules are detected using thresholding, and morphological operations, and extracted 3D skeletonization features that are given to the SVM classifier. When evaluated on the LIDC-IDRI database this method achieved a sensitivity of 89.3%. Saien [14], by assortment of 18 features detected nodules. This method achieves a sensitivity of 83.98% when evaluated on the LIDC-IDRI database. Liu [12], detected nodules using Spatial Fuzzy C-Means (SFCM) method, assorted 22 features, and performed classification using unsupervised method random forest. This method gives a sensitivity of 92.4% when evaluated on the LIDC database.

Table 2. Comparison with recent cnn architectures.

Author	Database	No. of Nodules	Sensitivity%	FP per scan
Jiang [16]	LIDC-IDRI	25723	80.06	4.7
Setio [19]	LIDC-IDRI	1186	85.4	1
Qi [11]	LUNA16	1186	87	4
Wang [18]	LIDC	893	92	NM
Li [9]	JSRT	NM	94	5
Proposed	LIDC-IDRI	1186	94.8	2.4

Where NM stands for Not Mentioned.

Comparison with the recent CNN techniques from the literature

Table 2 provides the comparison performance of the proposed CAD system with the popular CNN architectures used for lung nodule detection and false-positive reduction. Jiang [16], detected nodules based on patch-based deep learning architecture, multiscale Frangi filters are used for false-positive reduction. This approach when evaluated on the LIDC-IDRI database attained a sensitivity of 80.06% considering 25723 nodules from 1006 cases. Setio [19], detected nodules using ConvNets. For false positive reduction, nine 2D patches were extracted and fed to ConvNets. When evaluated on the LIDC-IDRI dataset considering 1186 nodules from 888 scans a sensitivity of 85.4% was attained. Qi [11], proposed three different 3D CNN architectures and achieved 87% sensitivity when evaluated on the LUNA16 database. Wang [18], proposed a CF-CNN model for nodule detection and attained a sensitivity of 92% on the LIDC database. Li [9], designed three CNNs with input patches of size 12×12 , 32×32 , and 60×60 respectively. This method is assessed on the JSRT database giving 94% sensitivity. Figure 8 shows the performance of the proposed model with different false positive reduction schemes from the literature in terms of sensitivity and false-positive per scan. Figure 9 shows the types of features used by authors in the literature.

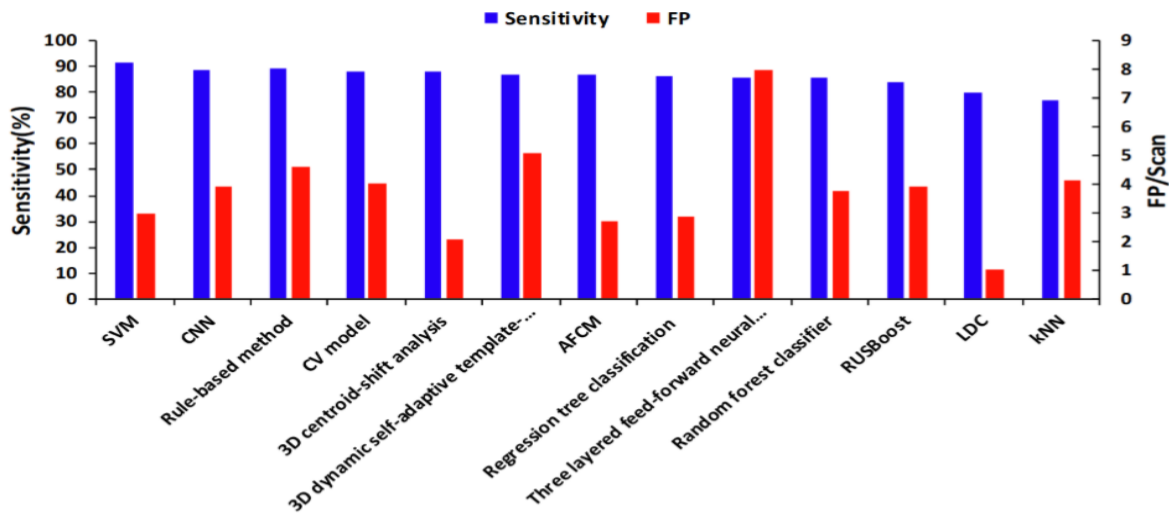


Fig. 8. Comparison with different false reduction schemes from the literature

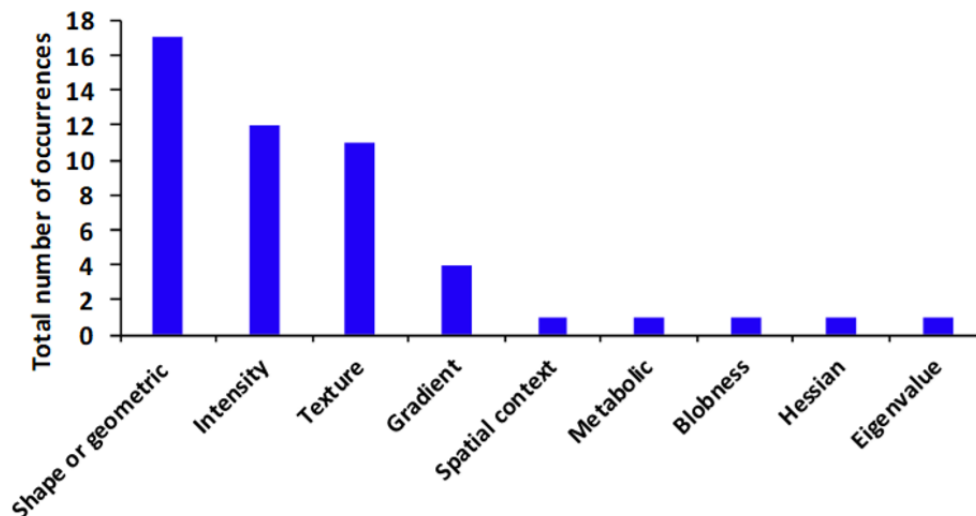


Fig. 9. Types of features used by different authors from the literature

Fig. 10 shows the nodules detected and missed by the proposed CADe system when operated 1FP/scan. The image patches are given in axial view (first row), sagittal image (second row), and coronal view (third row). The image patches are shown in 50×50 mm size with nodule centered.

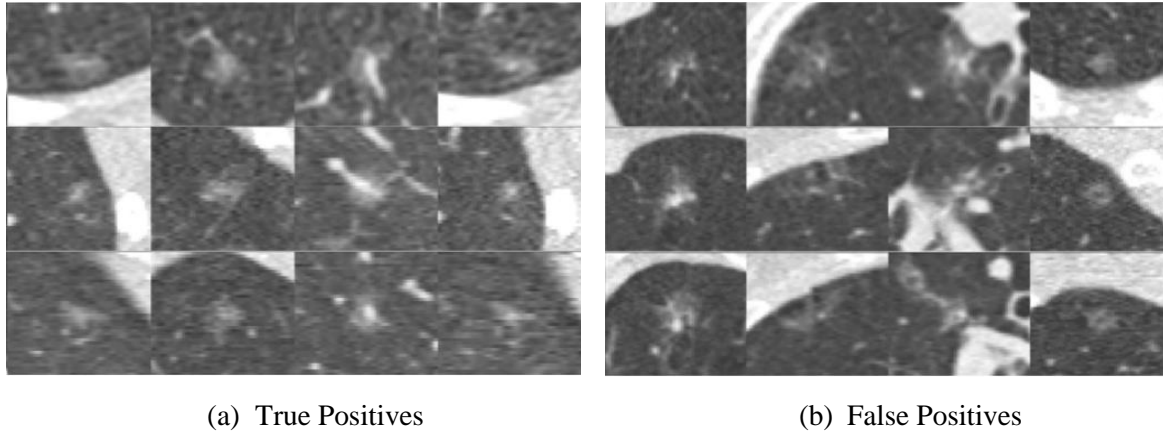


Fig. 10. Pulmonary Nodules detected representing a) True Positive nodules, and b) False Positive Nodules.

6. CONCLUSION

We proposed an efficient CADe system for the automatic detection of pulmonary nodules and the reduction of false positives (FP) per scan using patch-based Convolution Neural Networks (CNN). After detection of lung nodules, 64×64 image patches are drawn which are given as input to CNN. CNN is designed with three convolution layers, two maximum pooling layers and the last fully connected layer produces output such as nodule and non-nodule. The method when evaluated on the publicly available LIDC-IDRI database considering 888 scans with 1186 nodules, achieves 94.8% sensitivity, and 2.8 false positive (FP)/scan. The proposed CADe system shows promising results compared to recent techniques from the literature and proves CNN can be used for the early prediction of lung cancer. In the future, we will focus on 3D CNN's for the biopsy study of lung nodules.

REFERENCES

- [1] Siegel, Rebecca L., Kimberly D. Miller, and Ahmedin Jemal. "Cancer statistics, 2018." *CA: a cancer journal for clinicians* 68, no. 1 (2018): 7-30.
- [2] da Silva, Giovanni Lucca França, Thales Levi Azevedo Valente, Aristófanés Corrêa Silva, Anselmo Cardoso de Paiva, and Marcelo Gattass. "Convolutional neural network-based PSO for lung nodule false positive reduction on CT images." *Computer methods and programs in biomedicine* 162 (2018): 109-118.
- [3] Chen, Wanqing, Rongshou Zheng, Peter D. Baade, Siwei Zhang, Hongmei Zeng, Freddie Bray, Ahmedin Jemal, Xue Qin Yu, and Jie He. "Cancer statistics in China, 2015." *CA: a cancer journal for clinicians* 66, no. 2 (2016): 115-132.
- [4] Henschke, Claudia I., Dorothy I. McCauley, David F. Yankelevitz, David P. Naidich, Georgeann McGuinness, Olli S. Miettinen, Daniel M. Libby et al. "Early Lung Cancer Action Project: overall design and findings from baseline screening." *The Lancet* 354, no. 9173 (1999): 99-105.

- [5] Joyseeree, Ranveer, Sebastian Otálora, Henning Müller, and Adrien Depeursinge. "Fusing learned representations from Riesz Filters and Deep CNN for lung tissue classification." *Medical image analysis* 56 (2019): 172-183.
- [6] Hansell, David M., Alexander A. Bankier, Heber MacMahon, Theresa C. McLoud, Nestor L. Muller, and Jacques Remy. "Fleischner Society: glossary of terms for thoracic imaging." *Radiology* 246, no. 3 (2008): 697-722.
- [7] Prasoon, Adhish, Kersten Petersen, Christian Igel, François Lauze, Erik Dam, and Mads Nielsen. "Deep feature learning for knee cartilage segmentation using a triplanar convolutional neural network." In *International conference on medical image computing and computer-assisted intervention*, pp. 246-253. Springer, Berlin, Heidelberg, 2013.
- [8] Gupta, Anindya, Tonis Saar, Olev Martens, and Yannick Le Moullec. "Automatic detection of multisize pulmonary nodules in CT images: Large- scale validation of the false- positive reduction step." *Medical physics* 45, no. 3 (2018): 1135-1149.
- [9] Li, Chaofeng, Guoce Zhu, Xiaojun Wu, and Yuanquan Wang. "False-positive reduction on lung nodules detection in chest radiographs by ensemble of convolutional neural networks." *IEEE Access* 6 (2018): 16060-16067.
- [10] Zhang, Weihang, Xue Wang, Xuanping Li, and Junfeng Chen. "3D skeletonization feature based computer-aided detection system for pulmonary nodules in CT datasets." *Computers in biology and medicine* 92 (2018): 64-72.
- [11] Dou, Qi, Hao Chen, Lequan Yu, Jing Qin, and Pheng-Ann Heng. "Multilevel contextual 3-D CNNs for false positive reduction in pulmonary nodule detection." *IEEE Transactions on Biomedical Engineering* 64, no. 7 (2016): 1558-1567.
- [12] Liu, Ji-kui, Hong-yang Jiang, Chen-guang He, Yu Wang, Pu Wang, and He Ma. "An assisted diagnosis system for detection of early pulmonary nodule in computed tomography images." *Journal of medical systems* 41, no. 2 (2017): 30.
- [13] Gong, Jing, Ji-yu Liu, Li-jia Wang, Xi-wen Sun, Bin Zheng, and Sheng-dong Nie. "Automatic detection of pulmonary nodules in CT images by incorporating 3D tensor filtering with local image feature analysis." *Physica Medica* 46 (2018): 124-133.
- [14] S. Saien, H. A. Moghaddam, M. Fathian, A unified methodology based on sparse field level sets and boosting algorithms for false positives reduction in lung nodules detection, *International Journal of Computer Assisted Radiology & Surgery*, 13 (3) (2018) 397-409.
- [15] Taşçı, Erdal, and Aybars Uğur. "Shape and texture based novel features for automated juxtapleural nodule detection in lung CTs." *Journal of medical systems* 39, no. 5 (2015): 46.
- [16] Jiang, Hongyang, He Ma, Wei Qian, Mengdi Gao, and Yan Li. "An automatic detection system of lung nodule based on multigroup patch-based deep learning network." *IEEE journal of biomedical and health informatics* 22, no. 4 (2017): 1227-1237.
- [17] Han, Hao, Lihong Li, Fangfang Han, Bowen Song, William Moore, and Zhengrong Liang. "Fast and adaptive detection of pulmonary nodules in thoracic CT images using a hierarchical vector quantization scheme." *IEEE journal of biomedical and health informatics* 19, no. 2 (2014): 648-659.

- [18] Wang, Shuo, Mu Zhou, Zaiyi Liu, Zhenyu Liu, Dongsheng Gu, Yali Zang, Di Dong, Olivier Gevaert, and Jie Tian. "Central focused convolutional neural networks: Developing a data-driven model for lung nodule segmentation." *Medical image analysis* 40 (2017): 172-183.
- [19] Setio, Arnaud Arindra Adiyoso, Francesco Ciompi, Geert Litjens, Paul Gerke, Colin Jacobs, Sarah J. Van Riel, Mathilde Marie Winkler Wille, Matiullah Naqibullah, Clara I. Sánchez, and Bram van Ginneken. "Pulmonary nodule detection in CT images: false positive reduction using multi-view convolutional networks." *IEEE transactions on medical imaging* 35, no. 5 (2016): 1160-1169.
- [20] D. V. N. Sukanya, Giribabu. K, B. Prabhakar Rao, "Detection of Interstitial Lung Diseases from CT Scan Image", *Journal of Advanced Research in Dynamic Control Systems*, vol. 11, issue.3, pp. 1252-1260.
- [21] V. N. Sukanya Doddavarapu, Giri Babu Kande & B. Prabhakara Rao (2020) Differential diagnosis of Interstitial Lung Diseases using Deep Learning networks, *The Imaging Science Journal*, 68:3, 170-178, DOI: [10.1080/13682199.2020.1781394](https://doi.org/10.1080/13682199.2020.1781394)
- [22] Javaid, Muzzamil, Moazzam Javid, Muhammad Zia Ur Rehman, and Syed Irtiza Ali Shah. "A novel approach to CAD system for the detection of lung nodules in CT images." *Computer methods and programs in biomedicine* 135 (2016): 125-139.
- [23] Khordehchi, Elaheh Aghabalaee, Ahmad Ayatollahi, and Mohammad Reza Daliri. "Automatic lung nodule detection based on statistical region merging and support vector machines." *Image Analysis & Stereology* 36, no. 2 (2017): 65-78.
- [24] Teramoto, Atsushi, and Hiroshi Fujita. "Fast lung nodule detection in chest CT images using cylindrical nodule-enhancement filter." *International journal of computer assisted radiology and surgery* 8, no. 2 (2013): 193-205.
- [25] Abbas, Qaisar. "Segmentation of differential structures on computed tomography images for diagnosis lung-related diseases." *Biomedical Signal Processing and Control* 33 (2017): 325-334.
- [26] Setio, Arnaud AA, Colin Jacobs, Jaap Gelderblom, and Bram van Ginneken. "Automatic detection of large pulmonary solid nodules in thoracic CT images." *Medical physics* 42, no. 10 (2015): 5642-5653.
- [27] Firmino, Macedo, Giovanni Angelo, Higor Morais, Marcel R. Dantas, and Ricardo Valentim. "Computer-aided detection (CADe) and diagnosis (CADx) system for lung cancer with likelihood of malignancy." *Biomedical engineering online* 15, no. 1 (2016): 1-17.
- [28] Dhara, Ashis Kumar, Sudipta Mukhopadhyay, Anirvan Dutta, Mandeep Garg, and Niranjan Khandelwal. "A combination of shape and texture features for classification of pulmonary nodules in lung CT images." *Journal of digital imaging* 29, no. 4 (2016): 466-475.
- [29] Mukhopadhyay, Sudipta. "A segmentation framework of pulmonary nodules in lung CT images." *Journal of digital imaging* 29, no. 1 (2016): 86-103.
- [30] Li, Bin, Kan Chen, Guangming Peng, Yuanxing Guo, Lianfang Tian, Shanxing Ou, and Lifei Wang. "Segmentation of ground glass opacity pulmonary nodules using an integrated active contour model with wavelet energy-based adaptive local energy and posterior probability-based speed function." *Materials Express* 6, no. 4 (2016): 317-327.
- [31] Saien, Soudeh, Abdol Hamid Pilevar, and Hamid Abrishami Moghaddam. "Refinement of lung nodule candidates based on local geometric shape analysis and Laplacian of Gaussian kernels." *Computers in biology and medicine* 54 (2014): 188-198.

[32] Teramoto, Atsushi, Hiroshi Fujita, Osamu Yamamuro, and Tsuneo Tamaki. "Automated detection of pulmonary nodules in PET/CT images: Ensemble false- positive reduction using a convolutional neural network technique." *Medical physics* 43, no. 6Part1 (2016): 2821-2827.

[33] Chen, Bin, Takayuki Kitasaka, Hiroto Honma, Hirotsugu Takabatake, Masaki Mori, Hiroshi Natori, and Kensaku Mori. "Automatic segmentation of pulmonary blood vessels and nodules based on local intensity structure analysis and surface propagation in 3D chest CT images." *International journal of computer assisted radiology and surgery* 7, no. 3 (2012): 465-482.

[34] de Carvalho Filho, Antonio Oseas, Wener Borges de Sampaio, Aristofanes Correa Silva, Anselmo Cardoso de Paiva, Rodolfo Acatauassu Nunes, and Marcelo Gattass. "Automatic detection of solitary lung nodules using quality threshold clustering, genetic algorithm and diversity index." *Artificial intelligence in medicine* 60, no. 3 (2014): 165-177.

[35] Orozco, Hiram Madero, Osslán Osiris Vergara Villegas, Vianey Guadalupe Cruz Sánchez, Humberto de Jesús Ochoa Domínguez, and Manuel de Jesús Nandayapa Alfaro. "Automated system for lung nodules classification based on wavelet feature descriptor and support vector machine." *Biomedical engineering online* 14, no. 1 (2015): 9.